



1999

Gas Chromatography-Mass Spectrometry Analysis of 11-Nor-9-carboxy- Δ^9 -Tetrahydrocannabinol in Urine

Follow this and additional works at: <https://www.jfda-online.com/journal>

Recommended Citation

Lin, D.-L.; Kuo, T.-L.I.; and Liu, R.H. (1999) "Gas Chromatography-Mass Spectrometry Analysis of 11-Nor-9-carboxy- Δ^9 -Tetrahydrocannabinol in Urine," *Journal of Food and Drug Analysis*: Vol. 7 : Iss. 1 , Article 6.

Available at: <https://doi.org/10.38212/2224-6614.2884>

This Original Article is brought to you for free and open access by Journal of Food and Drug Analysis. It has been accepted for inclusion in Journal of Food and Drug Analysis by an authorized editor of Journal of Food and Drug Analysis.



Gas Chromatography-Mass Spectrometry Analysis of 11-Nor-9-carboxy- Δ^9 -Tetrahydrocannabinol in Urine

DONG-LIANG LIN^{1,2*}, TSUNG-LI KUO² AND RAY H. LIU³

¹ Scientific and Technical Research Center, Ministry of Justice Investigation Bureau, P.O. Box 3562, Taipei, Taiwan, R.O.C.

² Department of Legal Medicine, College of Medicine, National Taiwan University, Taipei, Taiwan, R.O.C.

³ Graduate Program in Forensic Science, University of Alabama at Birmingham, AL, 35294 U.S.A.

ABSTRACT

Effective specimen pretreatment and GC-MS protocols were developed for the analysis of 11-nor-9-carboxy- Δ^9 -tetrahydrocannabinol (THC-COOH) in urine. d_3 - and d_9 -11-nor-9-carboxy- Δ^9 -tetrahydrocannabinol (d_3 - and d_9 -THC-COOH) were evaluated as internal standards and conclusions were reached that THC-COOH can be effectively analyzed, qualitatively and quantitatively, as trimethylsilyl derivative using selective ion monitoring of the following ions: m/z 371, 473 and 488 (for THC-COOH) and m/z 380, 479 and 497 (for d_9 -THC-COOH). The extraction procedure achieved 90% recovery of the analyte in fortified drug-free urine containing 10-200 ng/ml THC-COOH. Using 2-ml sample size, the overall protocol resulted in the following analytical parameters in the 10-200 ng/ml concentration range studied: interday and intraday precision ranges, 0.35-5.31% and 0.44-5.19%, respectively; linearity, $r^2 > 0.999$.

Key words: GC-MS, internal standard, 11-nor-9-carboxy- Δ^9 -tetrahydrocannabinol, urine, drug of abuse.

INTRODUCTION

Overwhelming literature data resulting from a very significant number of studies have concluded that tetrahydrocannabinol (THC) is the most psychoactive constituent (ranging from trace to 12% in weight) in marijuana (*Cannabis sativa* L.)⁽¹⁾ and the detection of its metabolite, 11-nor-9-carboxy- Δ^9 -tetrahydrocannabinol (THC-COOH), in urine can be effectively used for monitoring marijuana exposure.

Several nondeuterated internal standards along with various specimen pretreatment procedures have been adopted for the analysis of THC-COOH in biological media^(2,3). d_3 -Analog has been the most popular choice when using GC-MS procedure, especially SIM mode was adopted⁽⁴⁻⁷⁾. Use of a d_6 -analog has also been reported in a recent study⁽⁸⁾.

This study critically evaluated potential interference among ions designated for monitoring THC-COOH and two candidates for internal stan-

dard, d₃- and d₉-THC-COOH. Selected ions were used along with the adopted pretreatment and other GC-MS parameters to study the effectiveness of the overall analytical procedure, in terms of recoveries, reproducibilities, assay linearity and detection limit.

MATERIALS AND METHODS

I. Reagents and Chemicals

All solvents were of HPLC grade and purchased from Baker (Phillipsburg, NJ). All reagents were of analytical grade and purchased from Merck (Darmstadt, Germany). *N*-Methyl-*N*-trimethylsilyltrifluoroacetamide (MSTFA) was obtained in 10-ml vials from Pierce Chemical (Rockford, IL). THC-COOH, d₃-THC-COOH, and d₉-THC-COOH were obtained from Radian Corporation (Austin, TX).

II. Extraction Procedure

Unless indicated otherwise, a typical analytical process utilizes 2 ml urine, which was first spiked with 50 μ l d₉-THC-COOH (2 μ g/ml in methanol) resulting in the inclusion of 100 ng (or 50 ng/ml) of the internal standard. Hydrolysis was then followed by adding 1 ml 2 N sodium hydroxide and 5 ml hexane containing 0.5% isoamyl alcohol, with the mixture placed on a low-speed shaker for 30 min at room temperature. Following 5 min centrifugation, the top organic layer was aspirated and the aqueous layer was transferred to a clean test tube, which was then added 0.5 ml 6 N HCl and pH checked (pH < 5). Five ml hexane/ethyl acetate (9:1, v/v) mixture was then added, followed by low-speed shaking for 15 min. The mixture was then centrifuged for 5 min and the top organic layer was transferred to a clean screw-top tube and evaporated to dryness at 50°C under a stream of nitrogen.

III. Preparation of Trimethylsilyl Derivatives

For derivatization, 75 μ l MSTFA was added to the residue in the screw-top tube prepared above. Capped tube was vortexed for 20 sec and

then heated at 100°C for 20 min. The reaction mixture was allowed to cool to room temperature prior to GC/MS analysis.

IV. Gas Chromatography-Mass Spectrometry Analysis

A Hewlett-Packard 5890 gas chromatography-5972 mass selective detector (GC-MS) equipped with an HP-G1034C Chemstation software was used for this study. The gas chromatograph was equipped with a 12-m Hewlett-Packard (Andover, MA) HP Ultra-1 (100% dimethyl polysiloxane phase) fused silica capillary column (0.20-mm ID; 0.33- μ m film thickness). The injector and interface temperature were maintained at 260°C and 280°C, respectively. Column oven temperature was held at 150°C for 1 min, then programmed to 300°C at 20°C/min, and held at the final temperature for 6.5 min. The following parameters were used for injecting samples into the GC-MS system: sample size, 3 μ l; injection mode, splitless; injector purge-off duration, 0.75 min.

V. Selection of Ions for Selective Ion Monitoring

THC-COOH and the two perspective internal standards were derivatized and analyzed using the procedure and parameters described above. Full-scan spectra of the derivatization products were first collected and examined for preliminary selection of candidate ions for collecting SIM data for qualitative and quantitative analysis purposes. SIM data of these ions were then collected to provide more definite information on cross-contributing the intensity of ions designated for the analyte by the perspective internal standard and vice versa.

RESULTS AND DISCUSSION

I. Selection of Deuterated Internal Standards and Ions

The full-scan spectra of THC-COOH (analyte) and its two deuterated analogs (d₃-THC-COOH and d₉-THC-COOH) were shown in Figure 1. The mass spectrum of d₉-THC-COOH

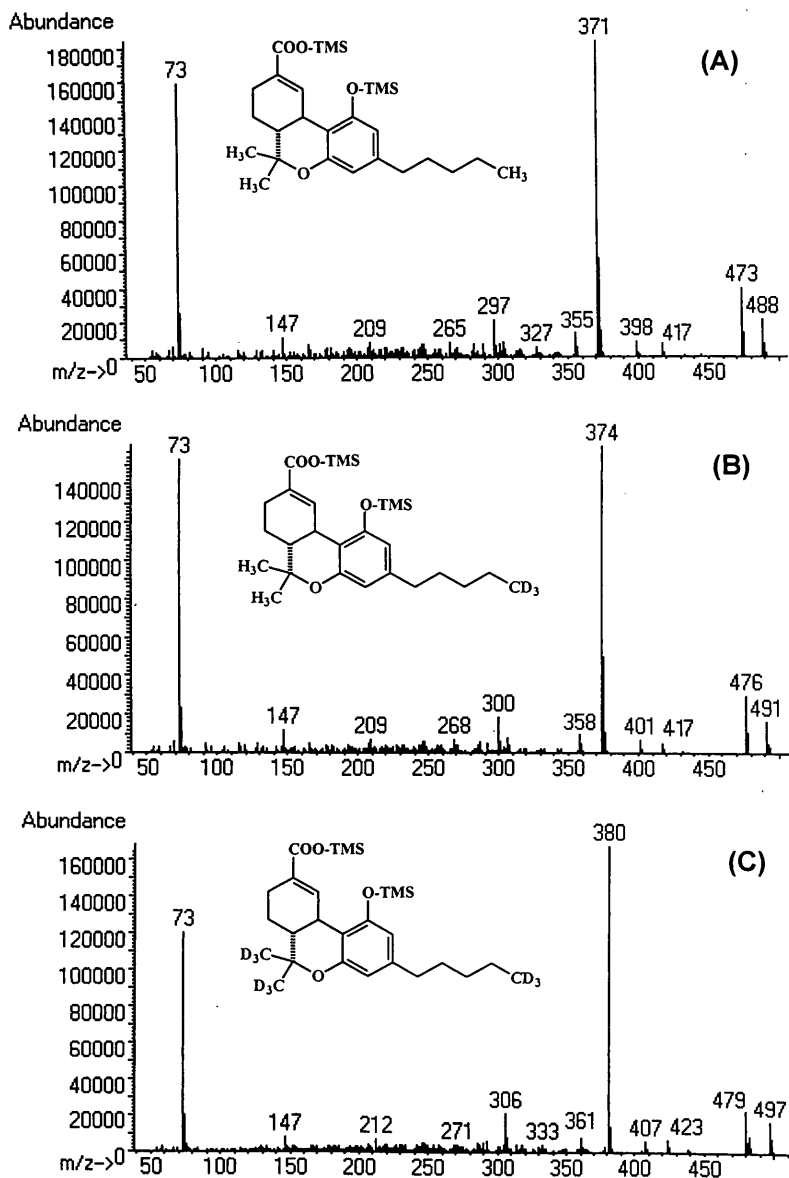


Figure 1. Full-scan mass spectra of TMS-derivatized THC-COOH (A), d₃-THC-COOH (B) and d₉-THC-COOH (C).

revealed relative intensities of 100%, 14.2%, and 10.5% at *m/z* 380, 479, and 497, respectively (Table 1). Since the full-scan mass spectrum of THC-COOH showed no peaks designated for these three ions (Table 1), indicated that it is free from interference by THC-COOH and can be designated for d₉-THC-COOH in SIM data acquisition. The full-scan mass spectrum of THC-COOH showed relative intensities of 100%, 21.7%, and 12.0% at *m/z* 371, 473, and 488, respectively

(Table 1). The absence of these ions in the full-scan mass spectrum of d₉-THC-COOH (Table 1) indicated no cross-contribution and being suitable for SIM data acquisition of THC-COOH. The data of SIM peak area integration (Table 2) indicated that all the cross-contributions to peaks at *m/z* 371, 473, 488 (designated for THC-COOH), 380, 479, and 497 (designated for d₉-THC-COOH) were 0%. These six ions appeared to be free from interference and being suitable for quantitation

Table 1. Relative intensity (in %) of selected ions from the full-scan mass spectra of TMS-derivatized THC-COOH, d₃- and d₉-THC-COOH

Ion (<i>m/z</i>)	THC-COOH	d ₃ -THC-COOH	d ₉ -THC-COOH
Ions designated for THC-COOH			
488	12.0	0.44	0
473	21.7	0.54	0
398	4.8	0.87	0
371	100	1.8	0
355	8.2	0.56	0.30
297	12.4	1.45	0.70
Ions designated for d ₃ -THC-COOH			
491	0	10.8	— ^a
476	0	19.3	—
401	0	4.74	—
374	0.46	100	—
358	0.48	6.74	—
300	1.00	11.9	—
Ions designated for d ₉ -THC-COOH			
497	0	— ^a	10.5
479	0	—	14.2
407	0	—	3.8
380	0	—	100
361	0	—	5.0
306	0.6	—	13.0

^aSince d₃- and d₉-THC-COOH will not be used together, the intensity data of these ions are irrelevant.

Table 2. SIM cross-contribution data of ion designated for the analyte and perspective internal standards

Deuterated analog	Analyte			Deuterated analog		
d ₃ -THC-COOH	488 (4.0%)	473 (3.3%)	398 (18%)	491 (0%)	476 (0%)	401 (0%)
	371 (1.6%)	355 (6.4%)	297 (13%)	374 (0.63%)	358 (9.5%)	300 (9.2%)
d ₉ -THC-COOH	488 (0%)	473 (0%)	398 (0%)	497 (0%)	479 (0%)	407 (0%)
	371 (0%)	355 (7.2%)	297 (6.3%)	380 (0%)	361 (11%)	306 (4.9%)

analysis.

The full-scan mass spectrum and SIM peak area integration data of d₃-THC-COOH/THC-COOH were shown in Table 1 and 2. Data in Table 2 indicated that cross-contribution to *m/z* 371, 473, 488 (designated for THC-COOH) and 374 (designated for d₃-THC-COOH) were 1.56%, 3.27%, 3.96% and 0.63%, respectively. Therefore,

d₉-THC-COOH is a preferable internal standard than d₃-THC-COOH for the quantitation of THC-COOH by GC/MS.

Relative intensity and cross-contribution data shown in Tables 1 and 2 indicated that selections of *m/z* 488, 473 and 371 (for THC-COOH) and *m/z* 497, 479 and 380 (for d₉-THC-COOH) provides ions that have significant intensities (> 10%)

with no cross-contribution interference. The most intense ions m/z 371 and 380 were used for quantification purposes. These ions were then used for the rest of this study.

II. Extraction Efficiency

Recoveries of the extraction procedure were studied by comparing the amount of the analyte (observed at the final GC-MS measuring step) in

Table 3. Extraction recoveries (%) of THC-COOH at different concentration (ng/ml) from fortified urine samples

Spiked conc.	Replicates	Mean \pm S.D. (%)
10	3	89.33 \pm 0.89
25	3	89.44 \pm 0.88
50	3	90.60 \pm 0.93
100	3	87.66 \pm 0.39
200	3	88.36 \pm 1.45

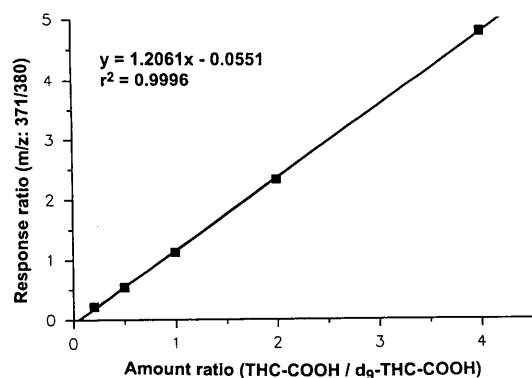


Figure 2. A typical calibration curve (10-200 ng/ml) for the analysis of THC-COOH using d_9 -THC-COOH as internal standard.

two sets of samples containing the same amount of the analyte. One set of these samples were proceeded with the extraction process, while the another set did not. Specifically, one set (Set I) of drug-free urine were spiked with THC-COOH stock (2 μ g/ml in methanol) to arrive at the following concentrations: 10, 25, 50, 100 and 200 ng/ml. Another set (Set II) of samples was prepared by spiking, into empty tubes, the corresponding amounts of THC-COOH stock (2 μ g/ml in methanol) used to prepare samples in Set I. Samples in set II were evaporated to dryness, while those in Set I were proceeded with the extraction process. The same amount of the internal standard was added to each sample in Set I and Set II immediately prior to the derivatization step.

Samples in both sets were then proceeded with identical derivatization and GC-MS analysis protocols. Amounts of the analyte in Set I was compared to that found in the corresponding samples in Set II. Resulting data are shown in Table 3. Approximately 90% recoveries were achieved.

III. Precision and Accuracy

To evaluate the precision of the overall analytical protocol, standard solutions of THC-COOH at 10, 25, 50, 100 and 200 ng/ml, each in triplicates, were prepared and analyzed for three times in one day (intraday study) and three times on three consecutive days (interday study). Results are shown in Table 4.

IV. Assay Linearity and Limit of Detection

A calibration curve based on the response

Table 4. Intraday and interday precision for analysis of urine fortified with THC-COOH

Spiked conc. (ng/ml)	Intraday			Interday		
	Mean ^a	Std dev	%CV	Mean ^a	Std dev	%CV
10	11.13	0.58	5.19	11.40	0.41	3.61
25	24.65	0.60	2.42	24.76	1.31	5.31
50	49.23	0.22	0.44	49.47	0.59	1.19
100	100.6	1.94	1.93	100.9	0.36	0.35
200	203.2	3.40	1.67	200.6	4.37	2.18

^aSample size: triplicates.

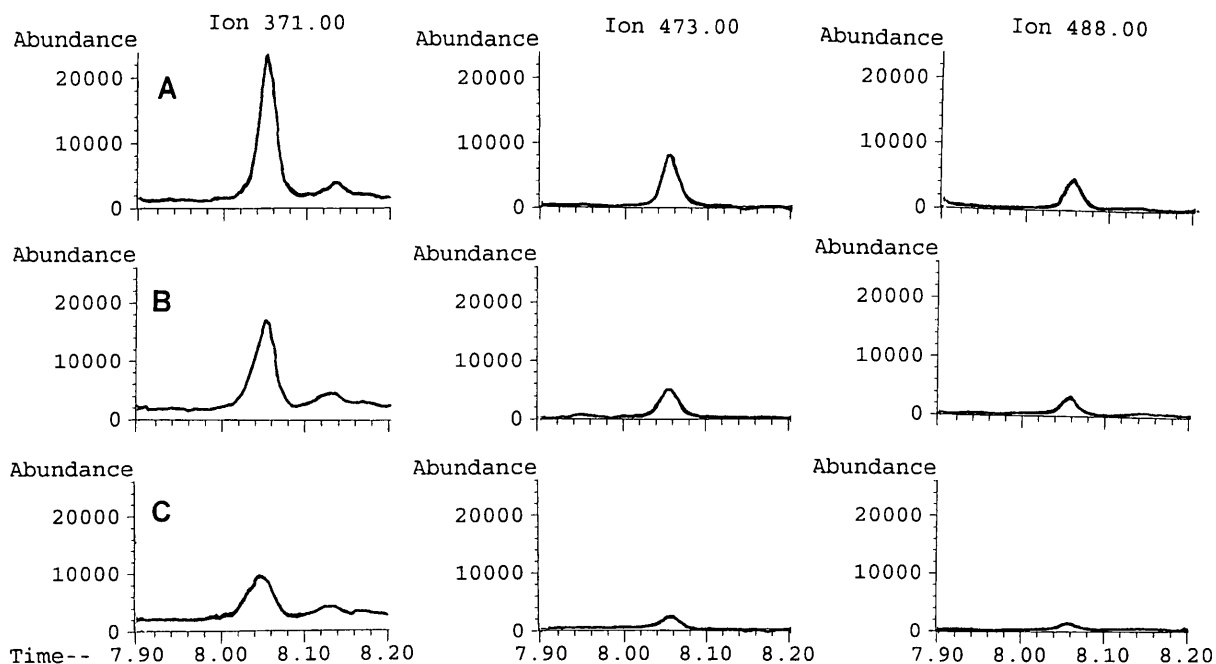


Figure 3. Ion chromatograms resulting from the analysis of 2-ml urine specimen spiked with 2.5 (A), 1.0 (B) and 0.5 (C) ng/ml THC-COOH.

ratios of quantification ions selected for THC-COOH and d_9 -THC-COOH (m/z 371 and 380, respectively) is shown in Figure 2. Assay protocol achieved excellent linearity within the 10-200 ng/ml concentration range studied: $r^2 > 0.999$. Ion intensity data shown in Figure 3 indicate the overall procedure can at least achieve 1 ng/ml detection limit.

In summary, d_9 -THC-COOH is an excellent internal standard, in terms of providing ions free of cross-contribution among ions designated for the analyte and the internal standard. Recovery, reproducibility, assay linearity, and detection limit data fully demonstrated the reliability of the protocol hereby reported.

ACKNOWLEDGMENT

Tsung-Li Kuo and Ray H. Liu are grateful to the National Science Council for financial supports (NSC 86-2811-M-002-001R- and NSC 86-2811-M-002-0026-) which facilitate the completion of this study.

REFERENCES

1. Baselt, R. C. and Cravey, R. H. 1995. Disposition of Toxic Drugs and Chemicals in Man. pp. 713-717. Chemical Toxicology Institute, Foster City, California, U.S.A.
2. ElSohly, M. A., ElSohly, H. N. and Jones, A. B. 1983. Analysis of the major metabolite of Δ^9 -tetrahydrocannabinol in urine II. An HPLC procedure. *J. Anal. Toxicol.* 7: 262-264.
3. ElSohly, M. A., Arafat, E. S. and Jones, A. B. 1984. Analysis of the major metabolite of Δ^9 -tetrahydrocannabinol in urine III. A GC/ECD procedure. *J. Anal. Toxicol.* 8: 7-9.
4. Karisson, L., Jonsson, J., Aberg, K. and Roos, C. 1983. Determination of Δ^9 -THC-11-oic acid in urine as its pentafluoropropyl-, pentafluoropropionyl derivative by GC/MC utilizing negative ion chemical ionization. *J. Anal. Toxicol.* 7: 198-202.
5. Paul, B. D., Mell, L. D., Mitchell, J. M., McKinley, R. M. and Irving, J. 1987. Detection and quantitation of urinary 11-nor- Δ^9 -

- tetrahydrocannabinol-carboxylic acid, a metabolite of tetrahydrocannabinol, by capillary gas chromatography and electron impact mass fragmentography. *J. Anal. Toxicol.* 11:1-5.
6. Parry, R. C., Nolan, L., Shirey, R. E., Wochob, G. D. and Gisch, D. J. 1990. Pretreatment of urine samples for the analysis of 11-nor- Δ^9 -tetrahydrocannabinol-9-carboxylic acid using solid-phase extraction. *J. Anal. Toxicol.* 14: 39-44.
7. Moeller, M. R., Doerr, G. D. and Warth, S. 1992. Simultaneous quantitation of delta-9-tetrahydrocannabinol (THC) and 11-nor-9-carboxy-delta-9-tetrahydrocannabinol (THC-COOH) in screen by GC/MS using deuterated internal standards and its application to a smoking study and forensic cases. *J. Forensic Sci.* 37: 969-983.
8. ElSohly, M. A., Little, T. L. and Stanford, D. F. 1992. Hexadeutero-11-nor- Δ^9 -tetrahydrocannabinol-9-carboxylic acid: A superior internal standard for the GC/MS analysis of Δ^9 -THC acid metabolite in biological specimens. *J. Anal. Toxicol.* 16:188-191.

以氣相層析質譜儀分析尿中大麻代謝物

林棟樑^{1,2*} 郭宗禮² 劉瑞厚³

1. 法務部調查局 台北縣新店市中華路74號

2. 臺大醫學院法醫學科

3. 美國阿拉巴馬州立大學刑事鑑識研究所

摘 要

本研究係以氣相層析質譜分析法來定量尿中大麻代謝物 11-nor-9-carboxy- Δ^9 -tetrahydrocannabinol (THC-COOH)。經評估 d_3 -與 d_9 -THC-COOH 二種內標準品後，發現 d_9 -THC-COOH 對尿中大麻代謝物並無任何干擾定量分析之離子，適合 GC/MS 做定量分析。本實驗採三甲基矽化 (trimethylsilyl) 衍生物，以離子監測法 (SIM, Selected Ion Monitoring) 來定量，監測離子 THC-COOH 為 m/z 371, 473, 488，內標準 d_9 -THC-COOH 為 m/z 380, 479, 497。以 2 ml 空白尿液配製濃度在 10 至 200 ng/ml 範圍內，其抽取回收率平均約為 90%，日間與日內精密度試驗，其變異係數分別為 0.35 ~ 5.31% 與 0.44 ~ 5.19%，並具有良好的線性關係 $r^2 > 0.999$ 。

關鍵詞：氣相層析質譜分析法，氘內標準品，尿中大麻代謝物，定量分析。